

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/366986887>

Crestal Bone and Soft Tissue Stability Surrounding Laser Microtextured Collar of Dental Implant; A 3-Year Clinical and Radiographic Evaluation

Article · February 2023

DOI: 10.31080/ASDS.2023.07.1552

CITATIONS

0

READS

36

3 authors:



Osama Rasras

Arab American University

1 PUBLICATION 0 CITATIONS

[SEE PROFILE](#)



Mahmoud Abu Taa

Arab American University

24 PUBLICATIONS 166 CITATIONS

[SEE PROFILE](#)



Ala Hassan A Qamheya

Arab American University

6 PUBLICATIONS 31 CITATIONS

[SEE PROFILE](#)

Some of the authors of this publication are also working on these related projects:



Periodontology and dental implantology [View project](#)



lithium disilicate [View project](#)



Crestal Bone and Soft Tissue Stability Surrounding Laser Microtextured Collar of Dental Implant; A 3- Year Clinical and Radiographic Evaluation

Osama Abdelrahman Rasras, Mahmoud abu ta'a and Ala Hassan A Qamheya*

Department of Dental Science, Faculty of Graduate studies, Arab American University, Ramallah, Palestine

*Corresponding Author: Ala Hassan A Qamheya, Department of Dental Science, Faculty of Graduate studies, Arab American University, Ramallah, Palestine.

DOI: 10.31080/ASDS.2023.07.1552

Received: December 19, 2022

Published: January 05, 2023

© All rights are reserved by Ala Hassan A Qamheya, et al.

Abstract

Objective: To evaluate marginal bone level (MBL) and clinical performance of dental implants with laser microtextured collar after three years of loading.

Material and Methods: Randomly selected were 24 patients (mean age \pm standard deviation [SD] 44.0 ± 11.1 years) who had dental implants in the dental center at the Arab American University in Ramallah, Palestine. 64 implants are necessary to achieve 99% confidence level with a margin of error 0.1mm. Periapical radiographs were taken for these dental implants immediately after loading and 3-years after loading. Crestal bone resorption was evaluated taking into consideration the attached gingivae width. Probing pocket depth and bleeding scores were also evaluated.

Results: After 3 years of loading, the crestal bone loss was 0.74 ± 1.06 SD. Probing pocket depth 3.73 ± 0.85 SD. Gingivitis index (Bleeding on probing 0.77 ± 0.86 SD). Plaque index 0.40 ± 0.76 SD. In addition, no significant differences ($P = 0.708$) related to the attached gingiva width and radiographic bone loss were observed.

Conclusion: Laser microtexturing of the collar of the dental implants provide stability of hard and soft tissue around dental implants. Nevertheless, it did not eliminate crestal bone resorption. Within the limits of this study, the laser microtexturing can stabilize the soft tissue regardless of the width of attached gingiva.

Keywords: Crestal Bone Loss; Laser- Microtextured Collar Dental Implants; Biologic Width; Peri-Implantitis; Micro Gap

Abbreviations

MBL: Marginal Bone Level; SD: Standard Deviation; PPD: Probing Pocket Depth

Introduction

Dental implants are the most suitable procedures to replace missing teeth [1]. Multiple clinical trials and scientific research have been done on dental implant materials and designs to enhance osseointegration and to produce ideal stability of crestal bone and soft tissue around dental implants [2,3]. These studies concentrated on the change and physical, topographical, mechanical, and chemical characteristics of the surface of the dental implants [4,5]. One of these surface treatments is laser Microtexturing, which can enhance soft and hard tissue integrity around dental implants [6-9].

In laser microtexturing technology, the surface of the coronal collar of the dental implant are designed by microgrooves which

were made using computer-controlled laser ablation techniques [6,10,11]. This technique can produce a connective tissue attachment that works as a barrier which prevents epithelial down growth and protect the crestal bone [6,12,13].

Many factors contribute to the crestal bone loss including implant surgery, micro gap, biological width, implant crest module, occlusal overload, and peri-implantitis [14-17]. Implant crest module received the highest magnitude of shear and rotational forces during function. This will produce crestal bone resorption with time [16,17]. In a three Dimensional finite element analysis in 2010, Wan-Ling Shen, et al. examined the influence of implant collar design on stress and strain distribution in the crestal compact bone. In his study, he evaluated different dental implants' collars (straight, divergent, and convergent collar designs). He found that the divergent collar design had the lowest stress and strain in the adjacent compact crestal bone followed by straight and convergent collars [18]. Additionally, the surface of the implant collar affected

the marginal bone stability. Recently, dental implant clinical trials are focusing on reducing or eliminating crestal bone loss. In the past, they used the machined collar dental implants. They thought it would be effective in preventing plaque and calculus accumulation. Studies have demonstrated that roughened collars were more retentive to crestal bone and provide more stability for the peri-implant tissue than the machined smoothed collars. The roughness value of the implant collar were adjusted to stabilize the blood clot; so bone integration followed [14,15]. Nevertheless, after the normal bone remodeling occurred, the exposed rough surface accumulated as oral biofilm which yields to mucositis and peri-implantitis. The moderate roughness value and the nano-topography of laser microchanells had no biofilm formation in comparison with other surfaces [19]. Consequently, the micro surface enhanced the soft tissue attachment and fibril orientation to protect the implant biologic width when this surface was exposed to soft tissue [20-22].

In this study, the clinical observation of laser microtextured surface was done in terms of marginal bone stability and soft tissue stability.

Material and Methods

Patient population

This retrospective clinical study was approved by the Helsinki Committee for ethical approval (Palestinian Health Research Council, Gaza, Palestine. Approval no: PHRC/HC/1085/22). The study was conducted on patients treated with dental implants at the dental center at the Arab American University, Palestinian Territories, and the implant prosthesis were delivered between March 2019 and August 2019. 24 patients (mean age ± standard deviation [SD] 44.0 ± 11.1 years) with 64 implants were selected randomly from patient files where the patients signed an informed consent form. Among the 24 patients, 14 were male and 10 were female. Most of the patients were non-smokers (18) table 1.

The patients included in this study have adhere to the following criteria: good oral hygiene, healthy patients without any systemic diseases, implant placed without bone augmentation, implant placed in complete healing sites, and at least 3 months passed after tooth extraction. Moreover, they have healthy adjacent teeth without periapical lesions and implants placed at the level of bone from the mesial and distal margins. In addition, the exclusion criteria include patients with any local or systemic disease, alcoholism, pa-

| | |
|-------------------|------------------|
| Gender | |
| Male, n (%) | 14 (58.3) |
| Female, n (%) | 10 (41.7) |
| Smoking status | |
| Smoker, n (%) | 6 (25.0) |
| Non-smoker, n (%) | 18 (75.0) |
| Age | |
| Mean ± SD | 44.0 ± 11.1 |
| Median | 42.0 |
| Range | 47.0 (70.0-23.0) |

Table 1: Patient population.

tients complaining from bruxism, patients complaining from untreated periodontal disease, and all implants placed sup or supra bone level were also excluded.

Marginal bone level (MBL)

MBL of dental implant was evaluated on Periapical radiograph taken at baseline (Implant Placement), at the time of prosthetic crown placement (3-4 months). A follow-up was done after 3 years. In addition, standard parallel periapical radiographs with film holder (KerrHawe SA) were taken by a phosphor plate (Xios scan, Sirona heliodent pluse). Sidexis software was used to measure the distance from the implant shoulder to the first visible bone contact of mesial and distal of the dental implants. All measurements were done by one investigator (O.R).

The MBL was measured as a linear distance from the margin of dental implant at the mesial and distal sides to the level of crestal bone margin, and the average of mesial and distal values were calculated.

Clinical parameters

All clinical parameters were investigated by one clinician (O.R). At patients recall (3 years after loading), the probing pocket depth (PPD) at the mesial, distal, buccal, and lingual surfaces of these dental implants was done by 1mm graduated perio-probe (Hu-Friedy). Plaque index scores were recorded according to the silness and loe index 1963 on all surfaces of the dental implants. Also, the Gingivitis index (bleeding index) scores were recorded according to the gingival index of Löe and Silness, 1963 [23]. Implant survival and success rates were also measured according to Albrektsson, et

al. 1986 [1,24,25]. The attached gingiva width were measured by Perio-probe (HuFriedy) from the gingival margin to the mucogingival line.

Statistical Analysis

Sample size calculation determined that 46 implants are necessary to achieve a 99% confidence level with a margin of error 0.1mm (Minitab®). The study’s clinical and radiographic variables were described by mean and standard deviation (SPSS V.23). Mann-Whitney U test was used for the comparison of MBL of attached gingiva ≥2mm surrounding implant and attached gingiva < 2mm.

Results

At the 3-year follow up, all 24 patients were available for radiographic (Figure 1) and clinical evaluation. All 64 implants were functional with a cumulative survival rate of 100% at the 3- year follow up. Based on the criteria of Albrektsson, the implants had a success rate of 93.84%. Additionally, the prosthesis were functional without chipping or complications.

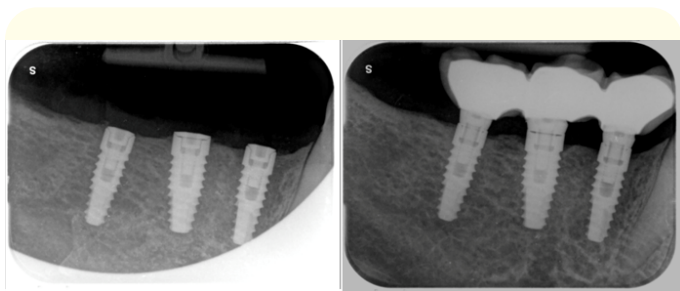


Figure 1: Peri-apical radiographs at implant placement day and 3 years after loading.

MBL

Table 2 summarizes the MBL change from the time of implant placement to the 36th month after loading. After 3 years of loading, the crestal bone loss was 0.74 ±1.06 SD. In 30 implants the average of marginal bone loss is 0-0.5m, while in 32 implants the average of marginal bone loss is 0.5-1mm. To add, at 7 implants the average of marginal bone loss is 1-1.5mm, and in 6 implants the marginal bone loss >1.5. No correlation was observed between implant site, smoking and sex with MBL. (Table 5)

| | Mean | Standard Deviation | Rang (Max-Min) | Median |
|---------------------------|------|--------------------|------------------|--------|
| Radiographic Crystal bone | 0.74 | 1.06 | -0.00)7.53 (7.53 | 0.00 |
| Mesial | 0.71 | 1.07 | -0.00)7.18 (7.18 | 0.00 |
| Distal | 0.77 | 1.09 | -0.00)7.36 (7.36 | 0.00 |

Table 2: Radiographic marginal bone loss after 3 years of loading.

Soft tissue parameters

The PPD, BI and PI were 3.73 ± 0.85, 0.77 ± 0.86, 0.40 ± 0.76 respectively (Table 3).

| | Mean | Standard Deviation | Rang (Max-Min) | Median |
|--|------|--------------------|-----------------|--------|
| Plaque index | 0.40 | 0.76 | 3.0 (3.00-0.00) | 0.00 |
| Probing pocket depth | 3.73 | 0.85 | 6.5 (7.50-1.00) | 3.75 |
| Gingivitis index (Bleeding on probing) | 0.77 | 0.86 | 2.0 (2.00-0.00) | 0.50 |

Table 3: Peri-implant soft tissue parameters after 3 years of loading.

No significant differences (P = 0.708) related to the attached gingiva width and radiographic bone loss were observed. (Table 4,5).

Discussion

According to previous studies, the mean of crestal bone loss around dental implants was 1.5mm after the first year of loading and 0.2 mm in every following year with a standard deviation of 0.3mm [24,26-28].

The results of this clinical and radiographic study showed 0.7 mm average marginal bone loss after 3 years of functional loading. Confirmatory results were also observed by Koodaryan., *et al*, where laser microtextured collar dental implants have significant crestal bone resorption reduction than machined collar dental implants. Moreover, he found a significant reduction in propping pocket depth around laser microtextured collar implants [29]. In another histologic study, the Laser Microchannels can produce connective tissue attachment with perpendicular collagen fibers resembling the tooth attachment which prevent epithelial down growth and crestal bone loss [10].

| Attached Gingiva Width | <2 | >2 | Test-statistic | p-value |
|---------------------------------|-------------|-------------|----------------|---------|
| Radiographic crestal bone level | 0.80 ± 1.35 | 0.69 ± 0.80 | 463.00 | 0.708 |

Table 4: Radiographic marginal bone loss according to the attached gingiva width.

| | Mean (Std. deviation) | Test statistic | p-value |
|-----------------------|-----------------------|----------------|---------|
| Gender | | -1.238 | 0.216 |
| Male | 0.77 (0.79) | | |
| Female | 0.70 (1.33) | | |
| Smoking status | | -0.320 | 0.749 |
| Smoker | 0.87 (1.46) | | |
| Non-smoker | 0.67 (0.74) | | |
| Arch | | -0.376 | 0.707 |
| Mandible | 0.86 (0.07) | | |
| Maxillae | 0.97 (1.87) | | |
| Number of implants | | -0.088 | 0.930 |
| Single implant | 1.00 (1.87) | | |
| Two adjacent implants | 0.67 (0.70) | | |

Table 5: Univariate analysis of marginal bone loss.

- Mann-Whitney U test was used to calculate significant levels (P value); cell value represents the percentage within the column (count).

Renzo Guarnieri, *et al.* evaluated 160 laser microtextured collar dental implants and 140 machined collars. The results of their research after 2 years support our study that a radiographical crestal bone resorption for test group is 0.58mm and for control group 1.09. Moreover, the clinical attachment loss was 0.55mm for the test group and 1.12mm for the control group [30].

Yojana B. Patil, *et al.* compared the crestal bone loss around implants with smooth collar and implants with micro threaded rough collar design. He found that Crestal bone loss adjacent to rough micro threaded-collar implants was significantly lower than smooth-collar implants [31]. Additionally, other studies that observe the laser micro structured collar in term of MBL and soft tissue stability were in line with our results [14,32,33].

Furthermore, Spyros Botos, *et al.* found that laser microtextured-collar dental implants have significantly shallower peri-implant pockets compared to machined collar. At a 6 and 12 month follow up the crestal bone loss adjacent to loaded laser microtex-

tured dental implants were (0.19mm and 0.42mm, respectively) and unloaded laser microtextured implants were (0.15mm and 0.29mm, respectively). For the control group (machined implants) at 6 and 12 months the crestal bone loss of loaded machined dental implants were (0.72 mm and 1.13 mm, respectively) and for the unloaded control group was (0.29mm and 0.55mm, respectively) [34].

Found in a study done by Gabriele E. Pecora, *et al.* in 2009, Laser-Lok surface treatment of dental implants reduced crestal bone resorption around the dental implant to 0.59 compared to 1.94 around machined dental surface implants, and probing pocket depth was of 2.30 mm versus 3.60 respectively [6].

Another study done by Linkevicius T, *et al.* compared laser-microtextured implants with platform switching implants according to crestal bone loss around them in thin peri-implant mucosa patients. They found that the laser microtexturing surface treated implant may produce less proximal bone loss than platform switching type in the pre-loading period. In the same study they found that those modalities in surface treatment of implants will not eliminate crestal bone resorption completely. Crestal bone loss of 0.71 and 1.02 was found in laser microtexturing and platform switching after 2 months respectively. At prosthesis delivery, it was 1.10 and 1.37 in laser microtexturing and platform switching, respectively. After a 1-year follow-up, the crestal bone loss was 1.41 and 1.43 in laser microtexturing and platform switching, respectively [35].

All the previous studies demonstrated good clinical and radiographical performance of laser microtextured collar dental implants. These results are comparable with our results.

The gingival biotype is the critical parameter that will influence the degree of crestal bone resorption and the stability of soft and hard tissue around dental implants [35]. In our study, when the attached gingiva is more than 2mm, there were no significant differences in MBL with those implants surrounded by less than 2mm of attached gingiva. This may be due to the limited numbers of implants incorporated in this study.

We cannot solely depend on bleeding upon probing to establish a diagnosis of peri implant condition, rather it needs multiclinical parameters like visual signs of inflammation (color changes, swelling, and suppuration), probing pocket depth and radiographical bone level around dental implants.

Conclusion

Within the limitations of this study, we can conclude that laser-microtextured collar dental implants provide stability of soft and hard tissue around it but do not prevent crestal bone loss completely.

Acknowledgements

No source of funding.

Conflict of Interest

Authors declare that there is no conflict of interest regarding the publication of this study.

Bibliography

1. Palmer R. "Introduction to dental implant". *British Dental Journal* 187 (1999): 127-132.
2. Anil S., et al. "Dental Implant Surface Enhancement and Osseointegration". *Implant Dentistry - A Rapidly Evolving Practice* (2011).
3. Souza JCM., et al. "Nano-scale modification of titanium implant surfaces to enhance osseointegration". *Acta Biomaterialia* 94 (2019): 112-131.
4. Raghavan R., et al. "Surface Treatments of Implant: A Review". *International Journal of Science and Healthcare Research* 5 (2020): 128.
5. Qamheya AHA., et al. "Thermal oxidation and hydrofluoric acid treatment on the sandblasted implant surface: A histologic histomorphometric and biomechanical study". *Clinical Oral Implants Research* 29 (2018): 741-755.
6. Pecora GE., et al. "Clinical evaluation of laser microtexturing for soft tissue and bone attachment to dental implants". *Implant Dentistry* 18 (2009): 57-66.
7. Guarnieri R., et al. "Influence of a Laser-Lok Surface on Immediate Functional Loading of Implants in Single-Tooth Replacement: Three-Year Results of a Prospective Randomized Clinical Study on Soft Tissue Response and Esthetics". *International Journal of Periodontics and Restorative Dentistry* 35 (2015): 865-875.
8. Farronato D., et al. "Influence of Laser-Lok Surface on Immediate Functional Loading of Implants in Single-Tooth Replacement: A 2-Year Prospective Clinical Study". *International Journal of Periodontics and Restorative Dentistry* 34 (2014): 79-89.
9. El Char E., et al. "Crestal Bone and Keratinized Tissue Around 3.0-mm Laser-Microtextured Dental Implants After 1 Year in Function: A Case Series". *International Journal of Periodontics and Restorative Dentistry* 39 (2019): 333-339.
10. Nevins M., et al. "Human histologic evidence of a connective tissue attachment to a dental implant". *International Journal of Periodontics and Restorative Dentistry* 28 (2008): 111-21.
11. Conserva E., et al. "Adhesion and proliferation of human dental pulp stem cells on a laser microtextured implant surface: an *in vitro* study". *Oral Health Care* (2018): 3.
12. Ketabi M and Deporter D. "The Effects of Laser Microgrooves on Hard and Soft Tissue Attachment to Implant Collar Surfaces: A Literature Review and Interpretation". *International Journal of Periodontics and Restorative Dentistry* 33 (2013): e145-e152.
13. Cary A Shapoff., et al. "Radiographic analysis of crestal bone levels around Laser-Lok collar dental implants". *The International Journal of Periodontics and Restorative Dentistry* 30.2 (2010): 129-137.
14. Randall E., et al. "The Effect of Dental Implant Collar Design on Crestal Bone Loss at 1 Year After Implant Placement". *International Journal of Periodontics and Restorative Dentistry* 39 (2019): 165-173.
15. Weiner S., et al. "The effects of laser microtextured collars upon crestal bone levels of dental implants". *Implant Dentistry* 17 (2008): 217-228.

16. Hagiwara Y. "Does platform switching really prevent crestal bone loss around implants?" *The Japanese Dental Science Review* 46 (2010): 122-131.
17. Oh T-J., et al. "The Causes of Early Implant Bone Loss: Myth or Science?" *Journal of Periodontology* 73 (2002): 322-333.
18. Shen WL., et al. "Influence of implant collar design on stress and strain distribution in the crestal compact bone: A three-dimensional finite element analysis". *The International Journal of Oral and Maxillofacial Implants* 25 (2010): 901-910.
19. Ionescu AC., et al. "Laser microtextured titanium implant surfaces reduce *in vitro* and *in situ* oral biofilm formation". *PLoS One* 13 (2018): 1-19.
20. Yanagisawa N., et al. "Human Gingival Fibroblast Attachment to Smooth Titanium Disks with Different Surface Roughnesses". *Biomimetics* 7 (2022): 164.
21. Doll PW., et al. "Enhancing the soft-tissue integration of dental implant abutments-*in vitro* study to reveal an optimized microgroove surface design to maximize spreading and alignment of human gingival fibroblasts". *Journal of Biomedical Materials Research Part B: Applied Biomaterials* 109 (2021): 1768-1776.
22. Quirynen M., et al. "Infectious risks for oral implants: a review of the literature". *Clinical Oral Implants Research* 13.200229 (2002): 1-19.
23. Augusta M., et al. "Gingival Diseases - Their Aetiology, Prevention and Treatment". *Gingival Diseases - Their Aetiology, Prevention and Treatment* (2012).
24. Karthik K., et al. "Evaluation of implant success: A review of past and present concepts". *Journal of Pharmacy and Bioallied Sciences* 5 (2013): S117.
25. Albrektsson T., et al. "The Long - Term Efficacy of Currently Used Dental Implants : A Review and Proposed Criteria of Success". *International Journal of Oral and Maxillofacial Surgery* 1 (1985): 11-25.
26. Cumbo C., et al. "Implant platform switching concept: A literature review". *European Review for Medical and Pharmacological Sciences* 17 (2013): 392-397.
27. Rocha S., et al. "Effect of platform switching on crestal bone levels around implants in the posterior mandible: 3 years results from a multicentre randomized clinical trial". *Journal of Clinical Periodontology* 43 (2016): 374-382.
28. Bryant SR and Zarb GA. "Crestal bone loss proximal to oral implants in older and younger adults". *Journal of Prosthetic Dentistry* 89 (2003): 589-597.
29. Koodaryan R and Hafezeqoran A. "Effect of laser-microtexturing on bone and soft tissue attachments to dental implants: A systematic review and meta-analysis". *Journal of Dental Research, Dental Clinics, Dental Prospects* 15 (2021): 290-296.
30. Guarneri R., et al. "The Impact of a Laser-Microtextured Collar on Crestal Bone Level and Clinical Parameters Under Various Placement and Loading Protocols". *The International Journal of Oral and Maxillofacial Implants* 29 (2014): 354-363.
31. Patil YB., et al. "Influence of Implant Neck Design on Crestal Bone Loss: A Comparative Study". *Nigerian Journal of Surgery: Official Publication of the Nigerian Surgical Research Society* 26 (2020): 22.
32. Chen Z., et al. "Influence of Laser-Microtextured Surface Collar on Marginal Bone Loss and Peri-Implant Soft Tissue Response: A Systematic Review and Meta-Analysis". *Journal of Periodontology* 88 (2017): 651-662.
33. Gultekin BA., et al. "Clinical Study Does the Laser-Microtextured Short Implant Collar Design Reduce Marginal Bone Loss in Comparison with a Machined Collar?" *BioMed Research International* (2016).
34. Botos S., et al. "The effects of laser microtexturing of the dental implant collar on crestal bone levels and peri-implant health". *The International Journal of Oral and Maxillofacial Implants* 26 (2011): 492-498.
35. Linkevicius T., et al. "Radiological comparison of laser-microtextured and platform-switched implants in thin mucosal biotype". *Clinical Oral Implants Research* 26 (2015): 599-605.